

Signa OpenSmart System Interconnect - 0.35T (FIXED SITE)


- 1 CUSTOMER FURNISHED
- 2 MAGNET POWER SUPPLIES ARE NOT INCLUDED WITH SYSTEM.
- 3 TYPICAL CONNECTION FOR NORMALLY CLOSED EMERGENCY OFF SWITCH
- 4 OPTIONAL: MAY NOT BE PRESENT ON ALL SYSTEMS
- 5 MAGNET RAMPING CABLES PASS THROUGH PP1 WITH PLATE REMOVED OR OPEN SCAN ROOM DOOR
- 6 CUSTOMER SUPPLIED TELEPHONE LINE FOR INSITE MODEM

*** Denotes a newly assigned run number for HFO
 1B D Denotes a newly assigned run number for MFO

CONTINUED ON NEXT PAGE →

Report updates for this diagram to Bruce Morton at Tel. (262) 521-6603

| | | | | |
|---------------------------|-----------|--------|-----|--------|
| MFO | | | | |
| Interconnect Diagram, MFO | | | | |
| SIZE | DATE | DWG NO | REV | |
| A3 | 06 Sep 00 | | A | |
| SCAL | NTS | SHEET | | 1 of 2 |
| T.Tsuchiya | | | | |

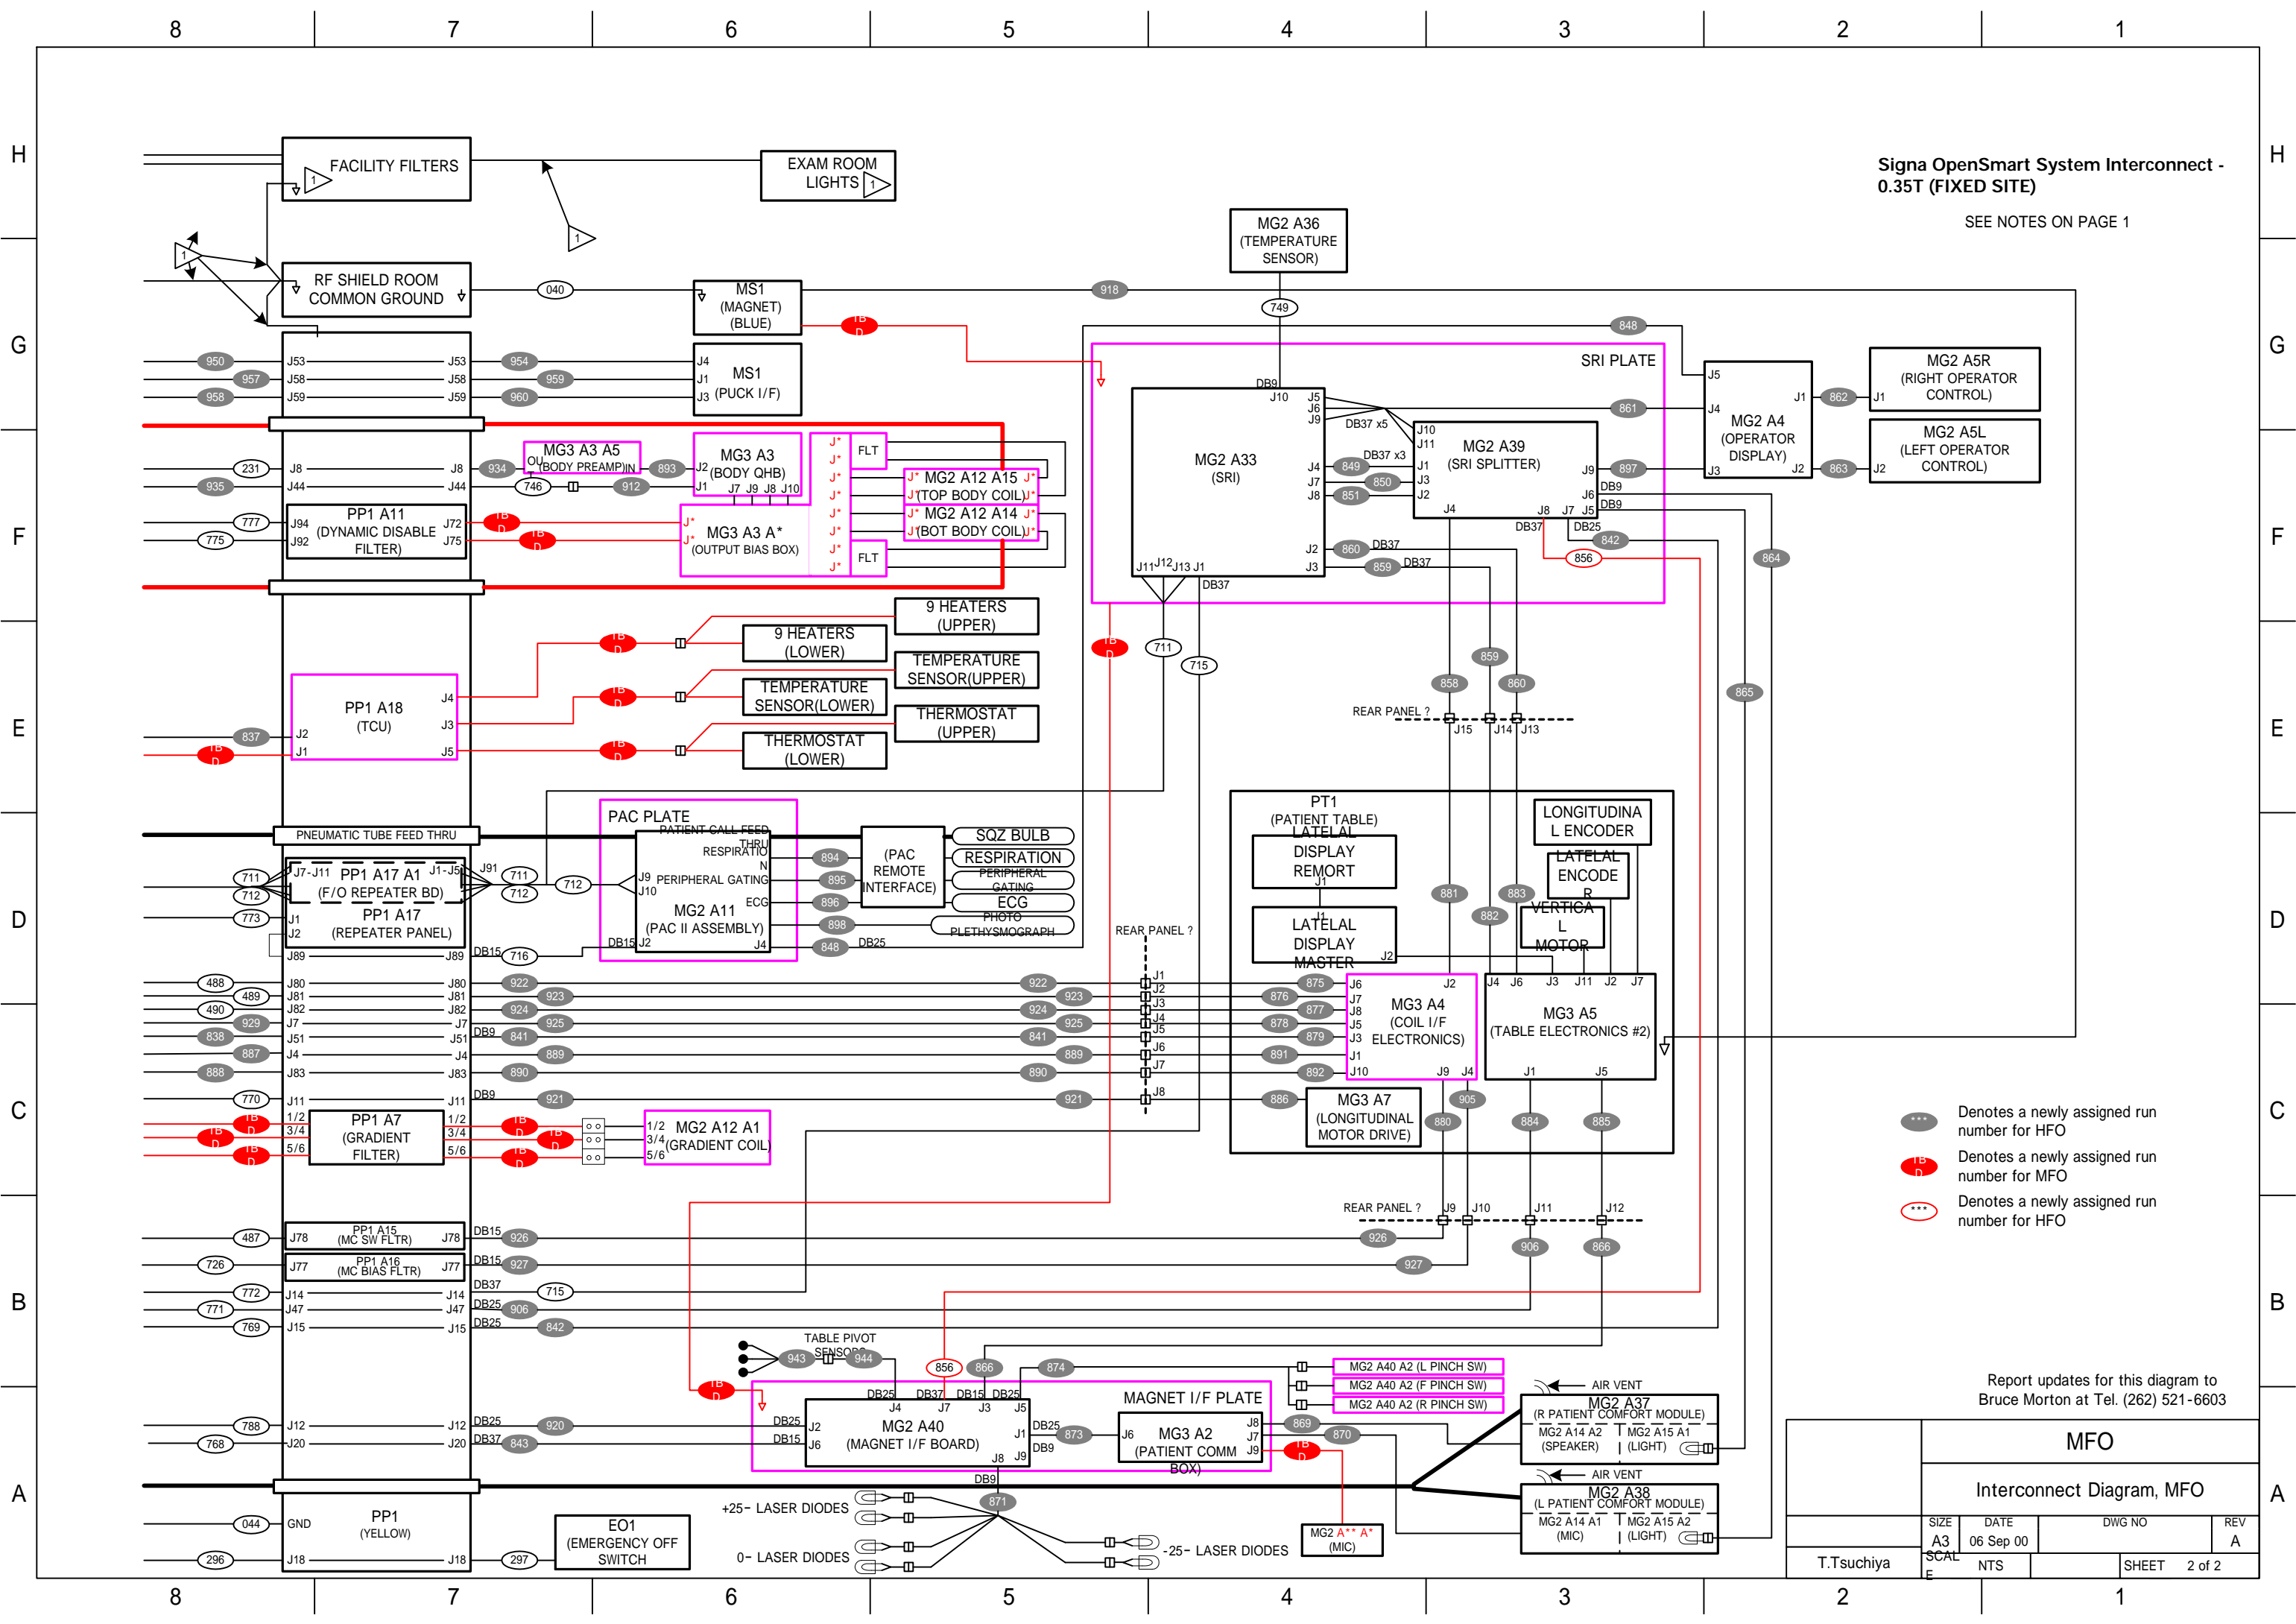

Signa OpenSmart System Interconnect - 0.35T (FIXED SITE)
SEE NOTES ON PAGE 1

- Denotes a newly assigned run number for HFO
- D Denotes a newly assigned run number for MFO
- Denotes a newly assigned run number for HFO

Report updates for this diagram to Bruce Morton at Tel. (262) 521-6603

| | | | |
|---------------------------|-------------------|--------|--------------|
| MFO | | | |
| Interconnect Diagram, MFO | | | |
| SIZE A3 | DATE 06 Sep 00 | DWG NO | REV A |
| T.Tsuchiya | SCAL E | NTS | SHEET 2 of 2 |

