

Signa Ovation System Interconnect - 0.35T (FIXED SITE)

- 1 CUSTOMER FURNISHED
- 2 TYPICAL CONNECTION FOR NORMALLY CLOSED EMERGENCY OFF SWITCH
- 3 MDP, EO1/E02 and RUN #296/#297 are used only high voltage.(over 380V)
- 4 RUN #1009 is connected to MDP, if exist.
- 5 OPTIONAL: MAY NOT BE PRESENT ON ALL SYSTEMS
- 6 CUSTOMER SUPPLIED TELEPHONE LINE FOR INSITE MODEM

● Denotes a newly assigned run number for HFO
 ● Denotes a newly assigned run number for MFO


CONTINUED ON NEXT PAGE →

Report updates for this diagram to T.Suzuki at Tel. +81-42-585-5951

Signa Ovation				
Interconnect Diagram, MFO				
APP. Y.Kato	SIZE A3	DATE 4 Sep 02	DWG NO 2353137SCH	REV 0
CH. S.Watanabe	SCALE	NTS	SHEET	1 of 2
DR. T.Suzuki				

Signa Ovation System Interconnect - 0.35T (FIXED SITE)

SEE NOTES ON PAGE 1

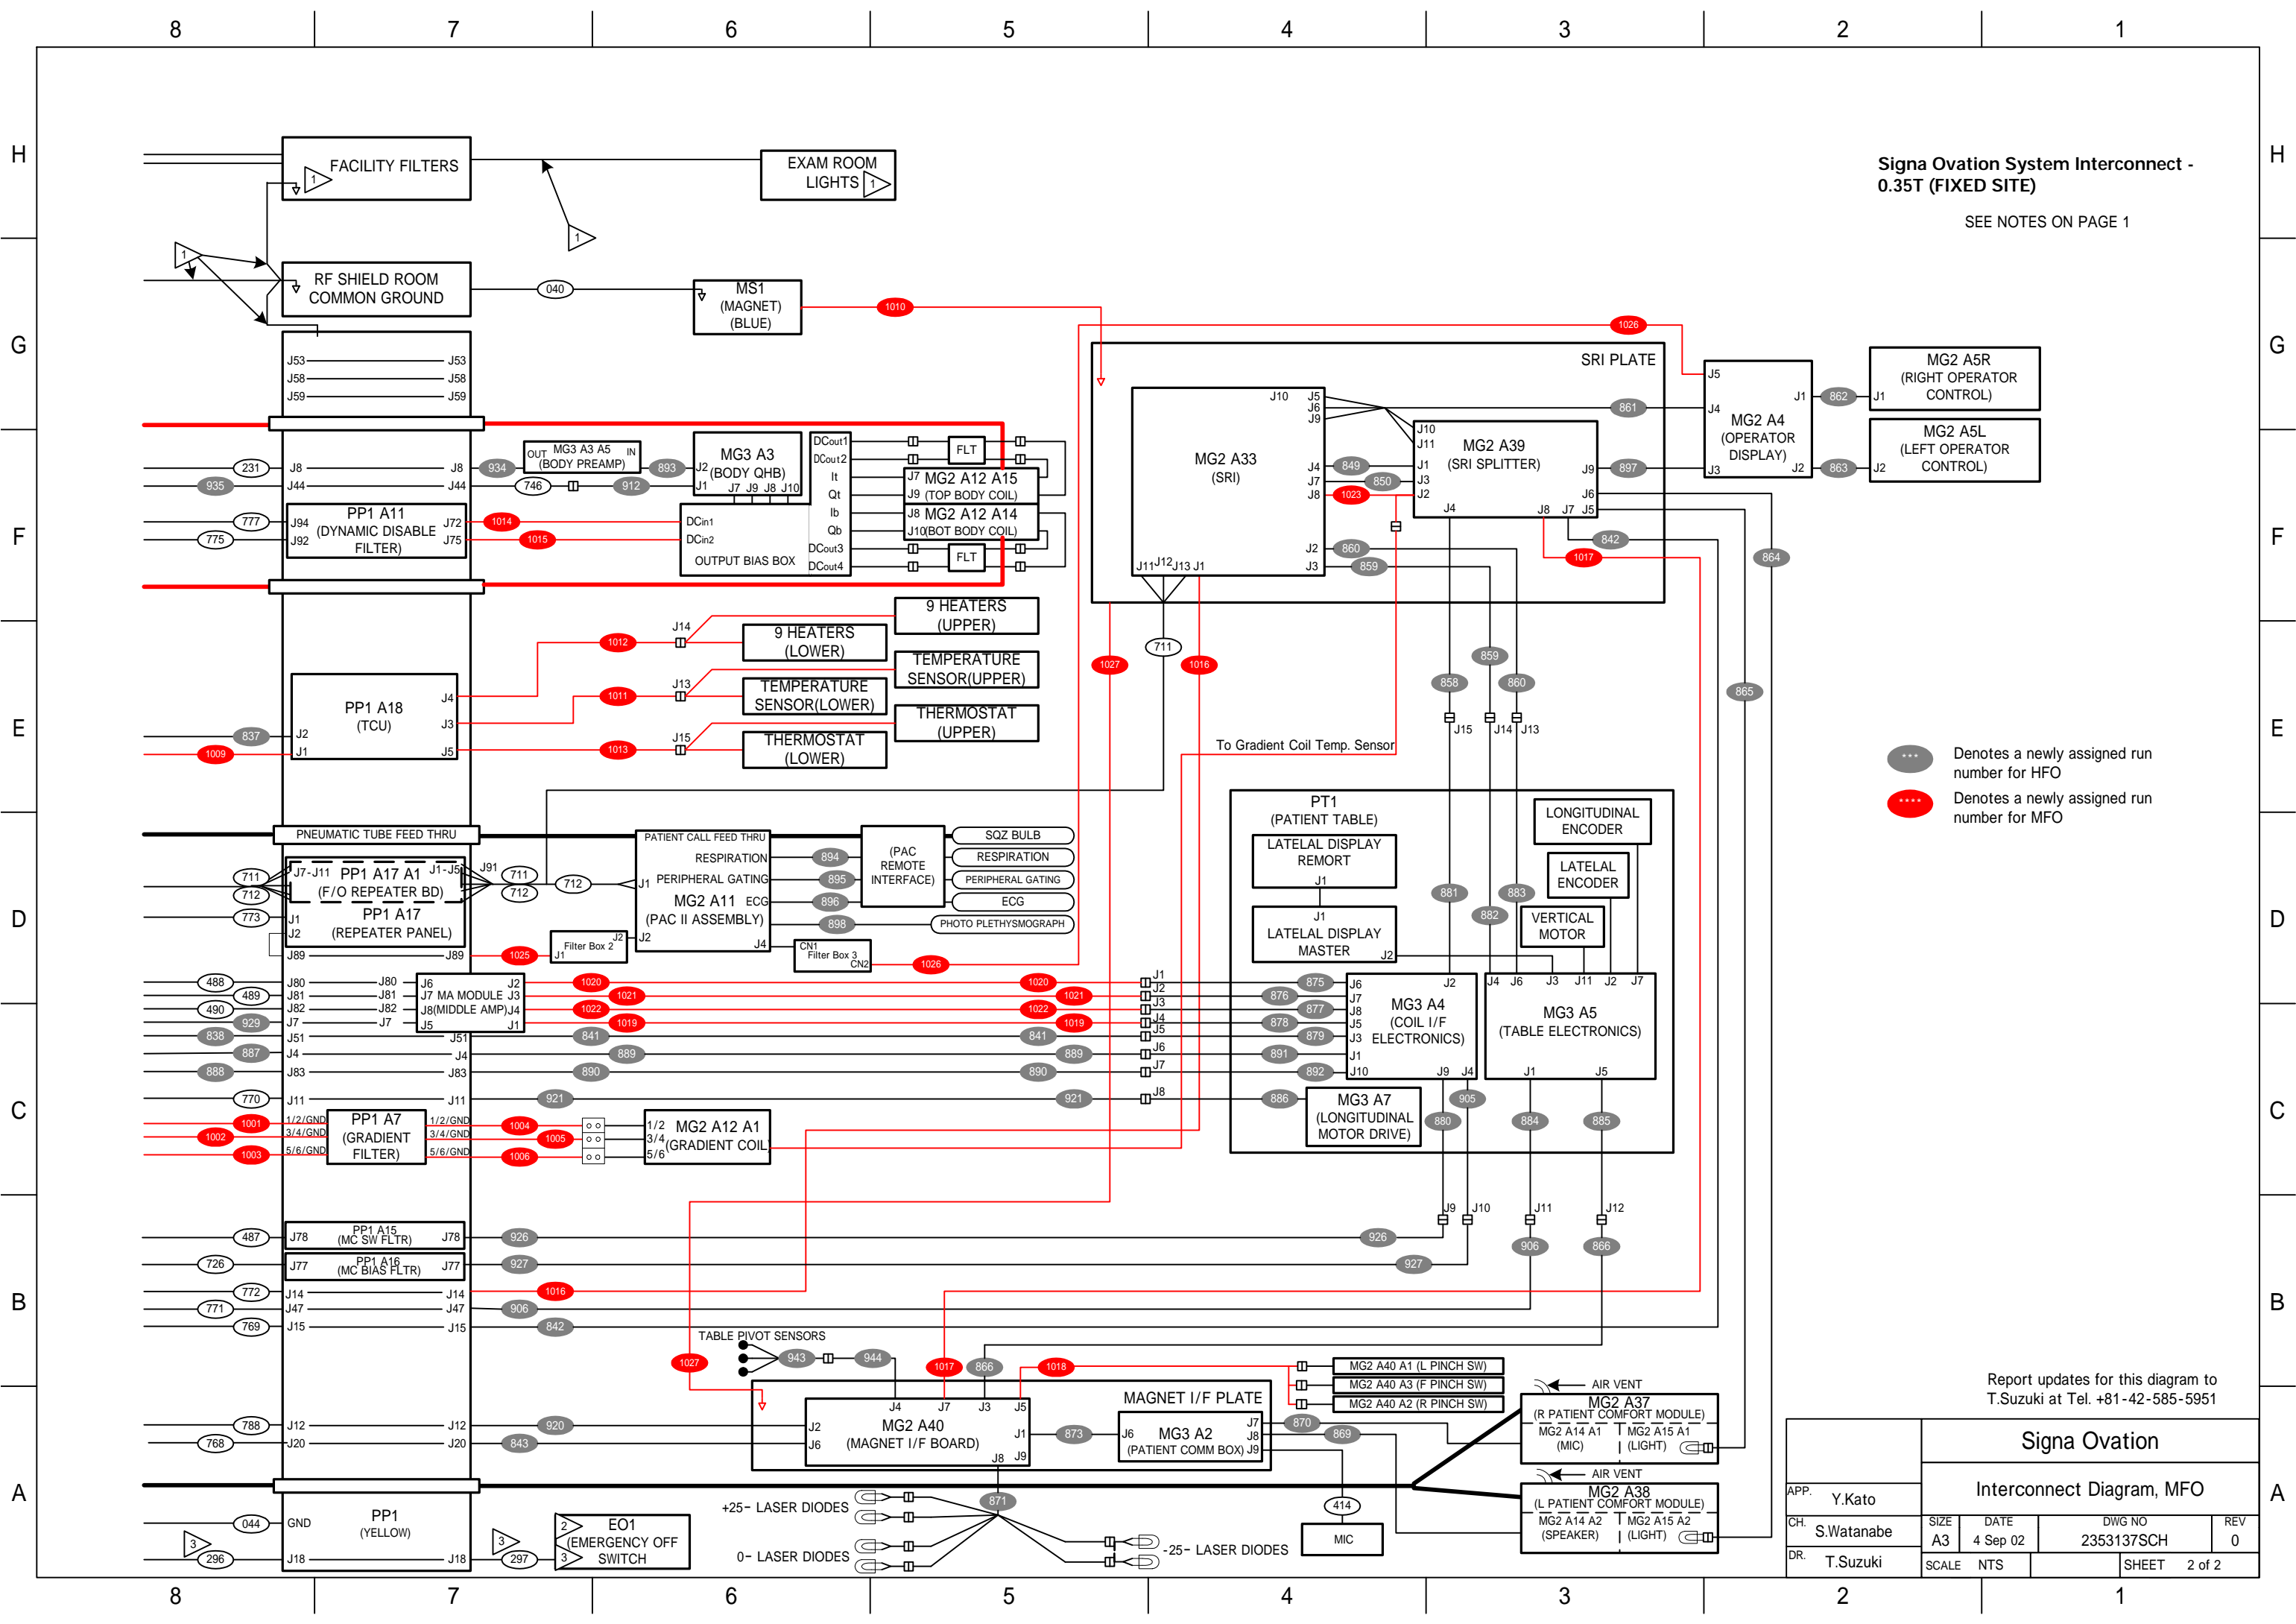

● Denotes a newly assigned run number for HFO
 ● Denotes a newly assigned run number for MFO

Report updates for this diagram to T.Suzuki at Tel. +81-42-585-5951

Signa Ovation									
Interconnect Diagram, MFO									
APP.	Y.Kato	SIZE	A3	DATE	4 Sep 02	DWG NO	2353137SCH	REV	0
CH.	S.Watanabe	SCALE	NTS			SHEET		2 of 2	
DR.	T.Suzuki								