

**Signa OpenSmart System Interconnect - 0.35T (FIXED SITE)**

- 1 CUSTOMER FURNISHED
- 2 MAGNET POWER SUPPLIES ARE NOT INCLUDED WITH SYSTEM.
- 3 TYPICAL CONNECTION FOR NORMALLY CLOSED EMERGENCY OFF SWITCH
- 4 OPTIONAL: MAY NOT BE PRESENT ON ALL SYSTEMS
- 5 MAGNET RAMPING CABLES PASS THROUGH PP1 WITH PLATE REMOVED OR OPEN SCAN ROOM DOOR
- 6 CUSTOMER SUPPLIED TELEPHONE LINE FOR INSITE MODEM

● Denotes a newly assigned run number for HFO  
 ● Denotes a newly assigned run number for MFO


CONTINUED ON NEXT PAGE →

Report updates for this diagram to Bruce Morton at Tel. (262) 521-6603

MFO				
Interconnect Diagram, MFO				
SIZE	DATE	DWG NO	REV	
A3	06 Sep 00		A	
SCAL	NTS	SHEET	1 of 2	
T.Tsuchiya				

Signa OpenSmart System Interconnect - 0.35T (FIXED SITE)

SEE NOTES ON PAGE 1

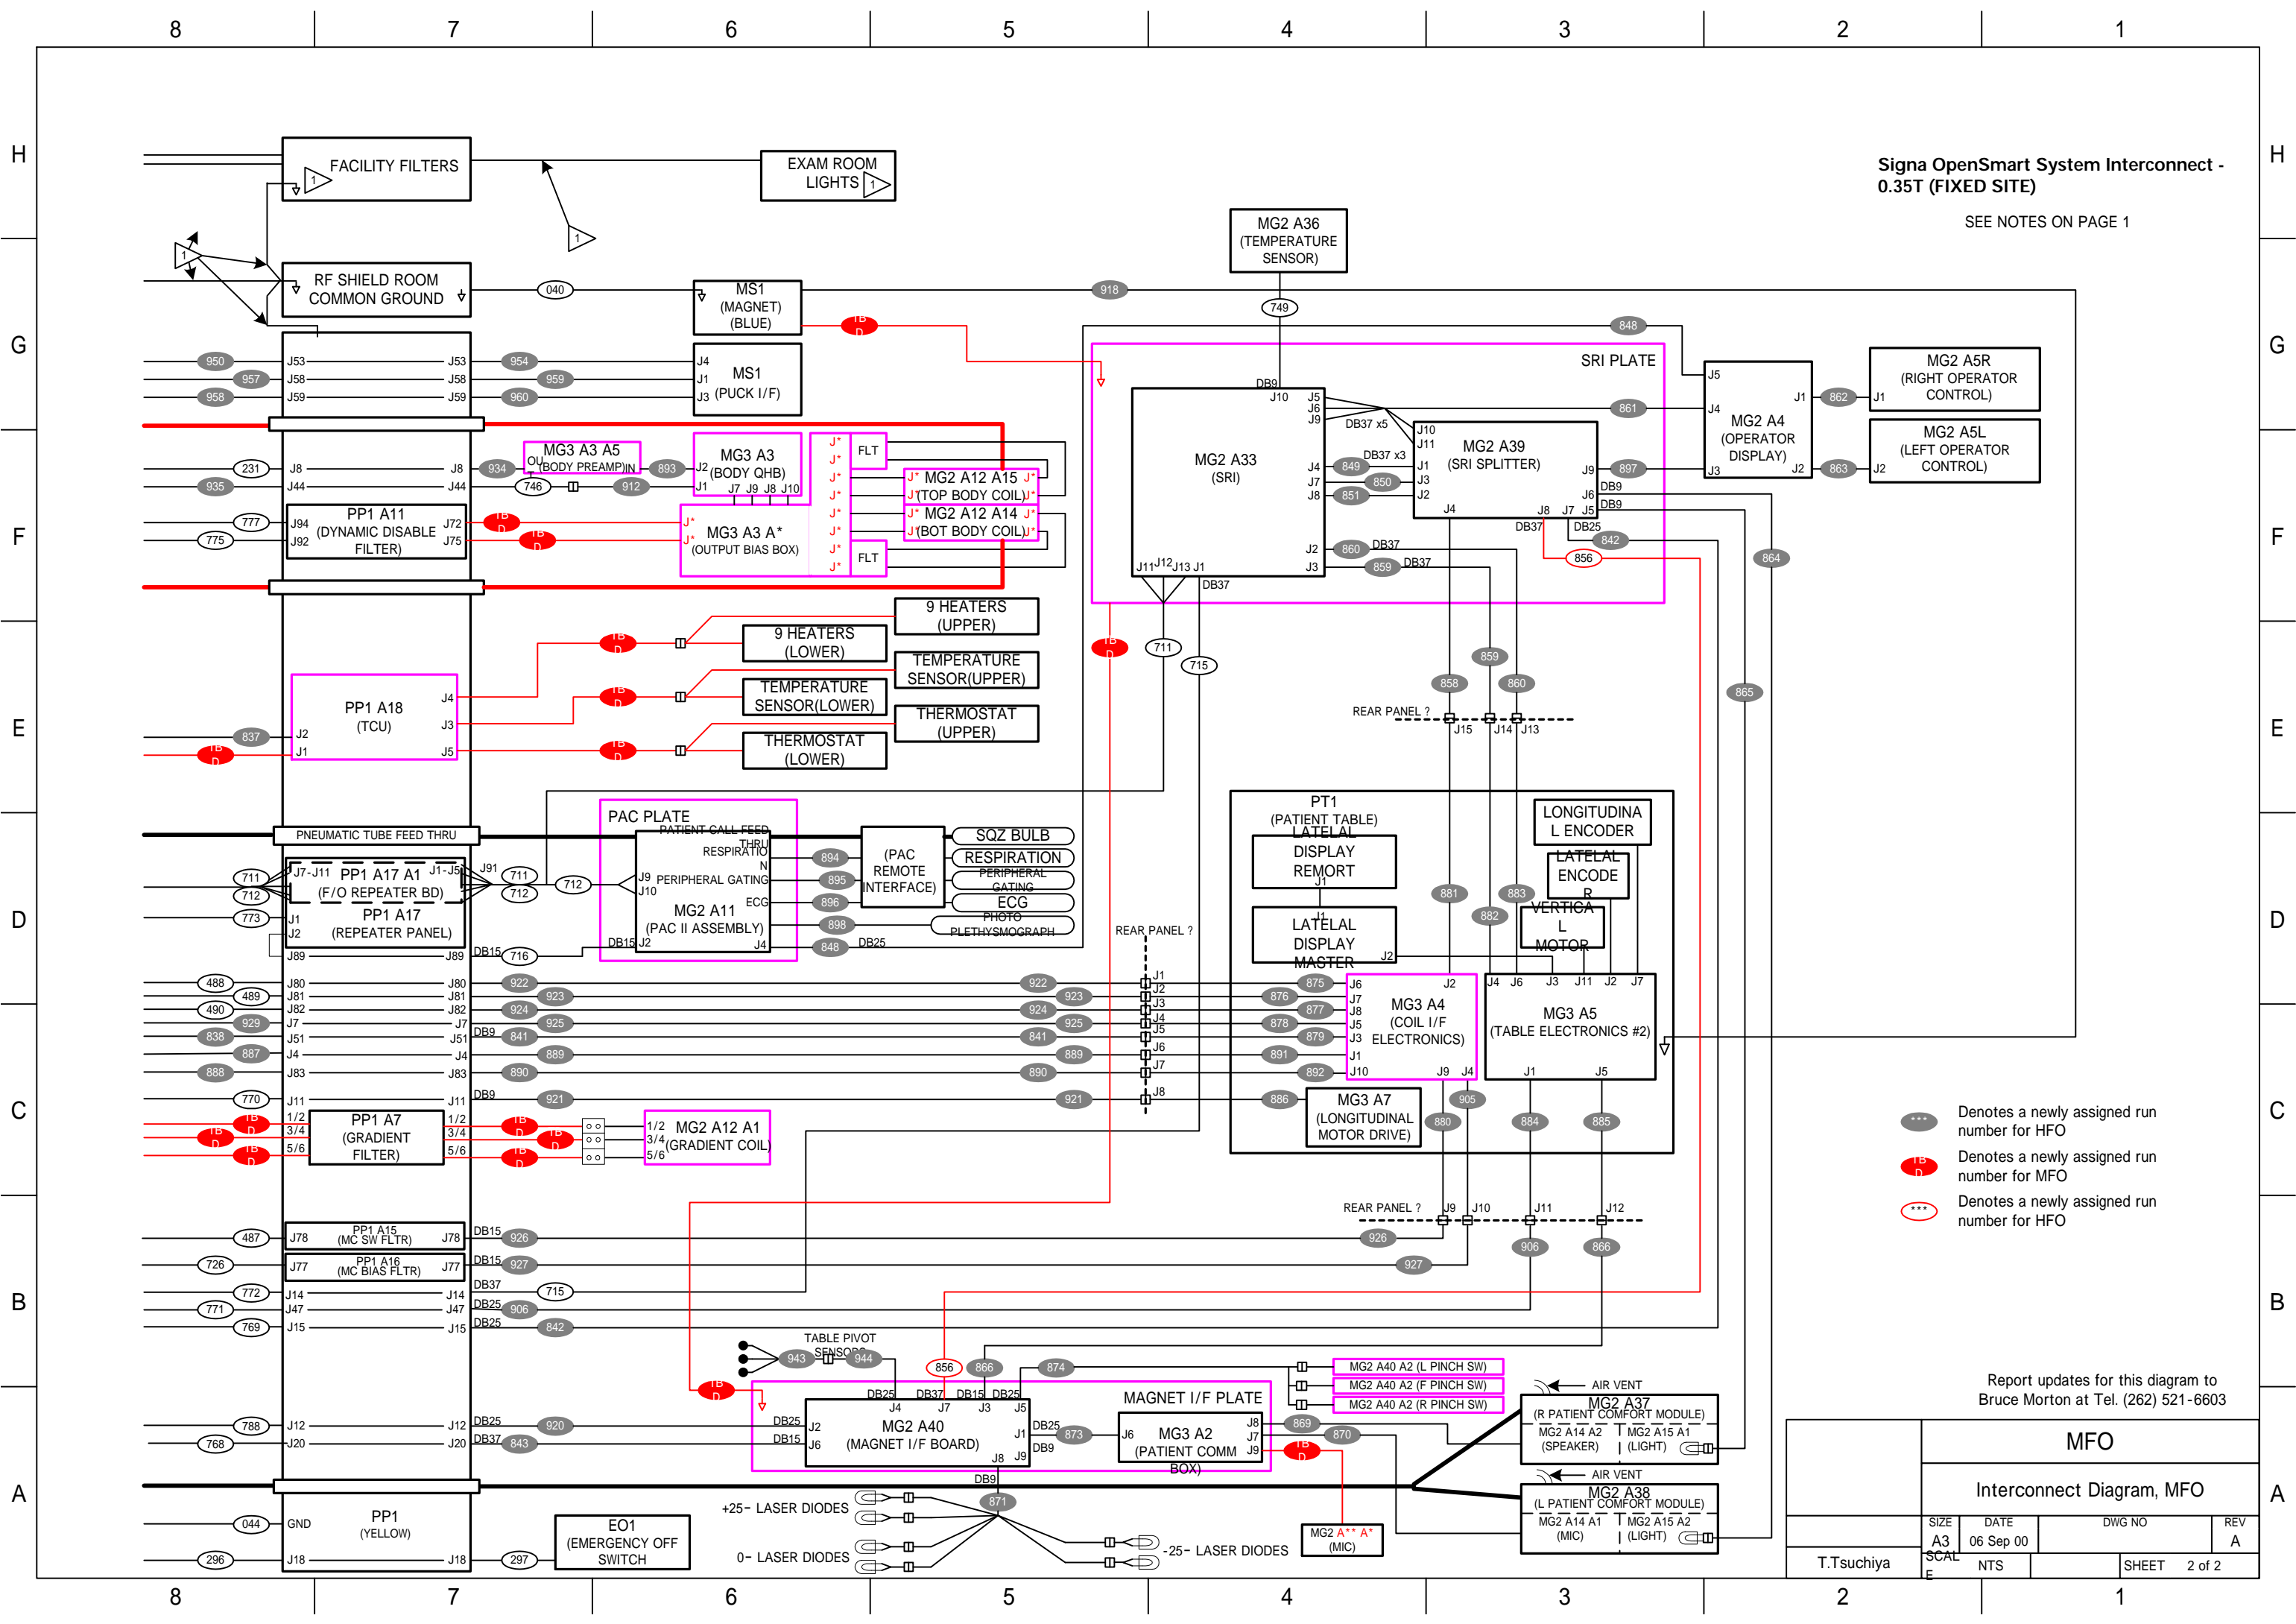

- ⦿ Denotes a newly assigned run number for HFO
- IB Denotes a newly assigned run number for MFO
- ⦿ Denotes a newly assigned run number for HFO

Report updates for this diagram to Bruce Morton at Tel. (262) 521-6603

MFO			
Interconnect Diagram, MFO			
SIZE A3	DATE 06 Sep 00	DWG NO	REV A
T.Tsuchiya	SCAL E	NTS	SHEET 2 of 2

